



# Carbon Monoxide Module

(Model No.: ZE16B-CO)

# Manual

Version: 1.2

Date of issue: 2023-3-27

Zhengzhou Winsen Electronics Technology Co., Ltd.

## Statement

This manual's copyright belongs to Zhengzhou Winsen Electronics Technology Co., LTD. Without the written permission, any part of this manual shall not be copied, translated, stored in database or retrieval system, also can't spread through electronic, copying, record ways.

Thanks for purchasing our product. In order to let customers use it better and reduce the faults caused by misuse, please read the manual carefully and operate it correctly in accordance with the instructions. If users disobey the terms or remove, disassemble, change the components inside of the sensor, we shall not be responsible for the loss.

The specific such as color, appearance, sizes &etc., please in kind prevail.

We are devoting ourselves to products development and technical innovation, so we reserve the right to improve the products without notice. Please confirm it is the valid version before using this manual. At the same time, users' comments on optimized using way are welcome.


Please keep the manual properly, in order to get help if you have questions during the usage in the future.

**Zhengzhou Winsen Electronics Technology CO., LTD.**

## Electrochemical Carbon Monoxide Gas Module ZE16B-CO

### Profile

ZE16B-CO is a general-purpose and miniaturization electrochemical carbon monoxide detection module. It utilizes electrochemical principle to detect CO in air which makes the module with high selectivity and stability. It is a combination of mature electrochemical detection principle and sophisticated circuit design.

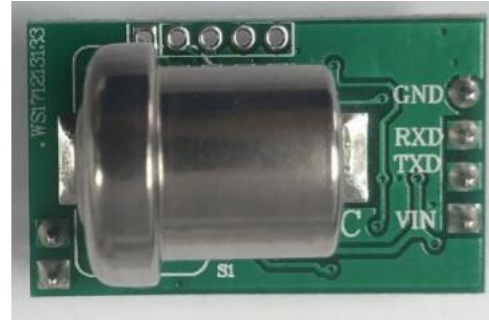

### Features


High sensitivity, fast response, good working stability, pre-calibrated

### Main Applications

Household CO alarm gas and CO detector.

### Technical Parameters Stable1.

Model No.	ZE16B-CO
Detection gas	Carbon Monoxide (CO gas)
Interfering gases	Alcohol &etc.
Output data	UART output 5V
Working voltage	5V DC
Preheating time	30 seconds
Response time	≤30 seconds
Recovery time	≤30 seconds
Detection range	0~500ppm
Solution	1ppm
Working temperature	-10°C~55°C
Working humidity	15%RH-90%RH (no condensation)
Storage temperature	-10°C~55°C
Life span	2 years (in air)

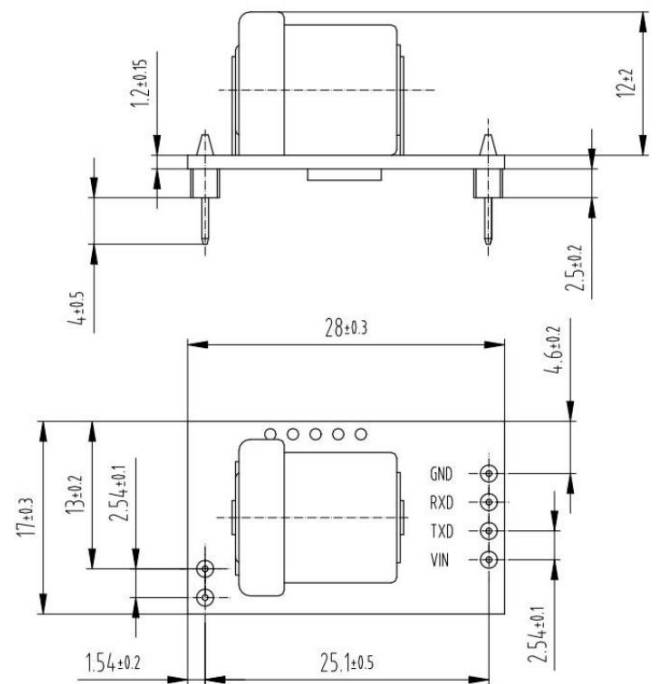


tolerance  $\pm 0.1\text{mm}$

**Fig1.** Structure

**Definition of pins Stable2.**

PIN1	PWM output 500ms is one period (20%~80% is corresponding 0~500ppm)
PIN2	Alarm status: high electrical level output if concentration $\geq 150$ ppm)
PIN3	GND
PIN4	UART (RXD)
PIN5	UART (TXD)
PIN6	VCC
NOTE: When the UART serial port is used, the PIN4 RX pin cannot hang in the air	

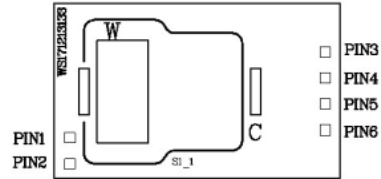

Stable2. Pins

**Communication Protocol**

**1. General Settings**

Table 3

Baud Rate	9600
Data bits	8
Stop Bits	1
Parity	None

**2. Communication Commands**

The communication is initiative upload mode, concentration value is sent every other 1s, command line as follow (300ppm concentration): **Table 4**

Byte0	Byte1	Byte2	Byte3	Byte4	Byte5	Byte6	Byte7	Byte8
Start Byte	Gas Type	Unit	No. of decimal	Concentration (High Byte)	Concentration (Low Byte)	Full Range (High Byte)	Full Range (Low Byte)	Check sum
0xFF	CO=0x04	ppm=0x03	0 byte=0x00	0x01	0x2C	0x01	0xF4	0xD7

Gas concentration value = High Byte\*256+Low Byte

So, CO concentration= 1x256+44=300 ppm

Full range = High Byte of full range \*256 + Low Byte of full range

**3. Check sum and calculation**

Check = (negation(byte1+bye2+.....+byte7))+1

Please refer the following example:

```

unsigned char FucChecksum(unsigned char *i,unsigned char ln)
{
    unsigned char j,tempq=0;
    i+=1;
    for(j=0;j<(ln-2);j++)
    
```

```
{  
    tempq+=*i;  
    i++;  
}  
tempq=(~tempq)+1;  
return(tempq);  
}
```

## Installation

This module adopts Pin2.54mm\*4 and Pin2.54mm\*2 single row pin structure for external connection. It is just need to weld the positioning needle to the fixed connection and the welding is manual mode.

## Cautions

1. DO NOT insert or extract the sensor on the PCB board.
2. DO NOT change or move the electronic part on the module.
3. Avoid sensor contact with organic solvent, coatings, medicine, oil and high concentration gases.
4. Excessive impact or vibration should be avoided.
5. Please keep the modules warming up for at least 20 minutes when first using.
6. Please do not use the modules in systems which related to human being's safety.
7. Please do not use the modules in strong air convection environment.
8. Please do not expose the modules in high concentration organic gas for a long time.

**Zhengzhou Winsen Electronics Technology Co., Ltd**

**Add:** No.299, Jinsuo Road, National Hi-Tech Zone,  
Zhengzhou 450001 China

**Tel:** +86-371-67169097/67169670

**Fax:** +86-371-60932988

**E-mail:** sales@winsensor.com

**Website:** www.winsen-sensor.com

